

CryoPen[®]


Innovating cryosurgery.
Empowering practitioners.






- The penetration rate of freezing with the CryoPen is approximately **1mm per 3 seconds** with a maximum freezing depth of **3 to 6mm** depending on the used applicator.
- The duration of the treatment time will depend on the surface area and the thickness of the tissue being treated.
- The closer you approach the lesion, the more freezing power you apply to the tissue.




- Recommended treatment session
 - **PRE FREEZE**
 - **FREEZE - THAW – FREEZE - THAW**
- Tissue must be allowed to thaw (defrost) for about 30 seconds between freeze sessions
- Note that the tissue will freeze faster in the second freeze and a shorter application may be sufficient
- **'freeze-thaw-freeze'** technique seems to offer the best opportunity for success

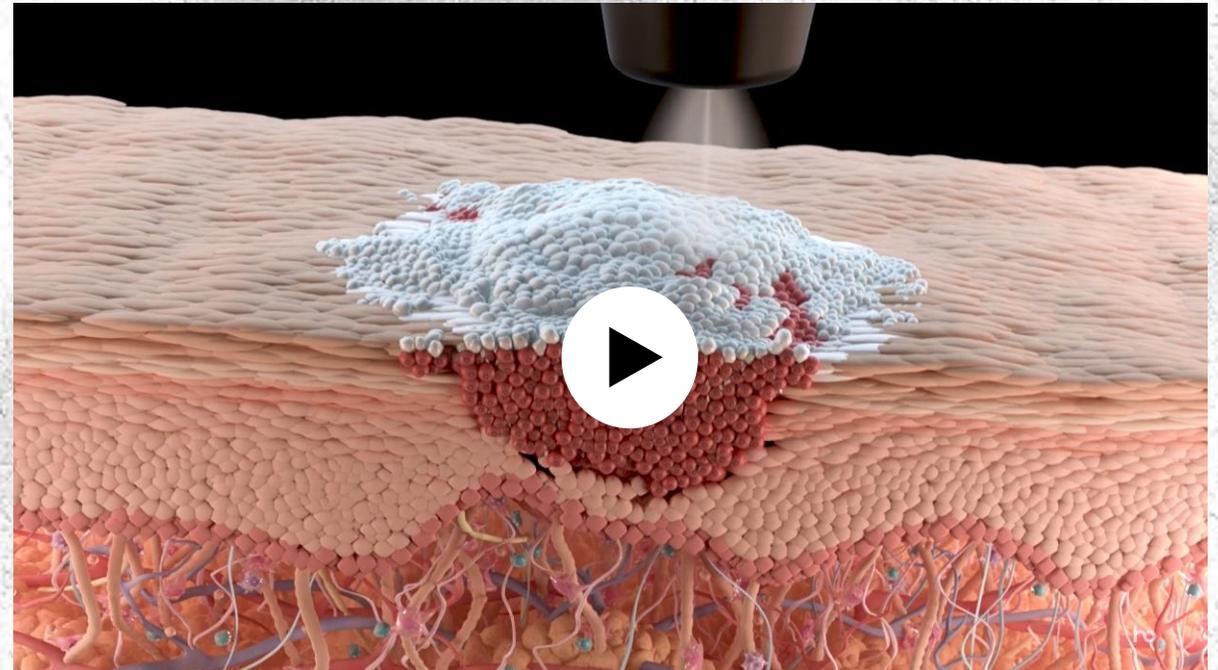





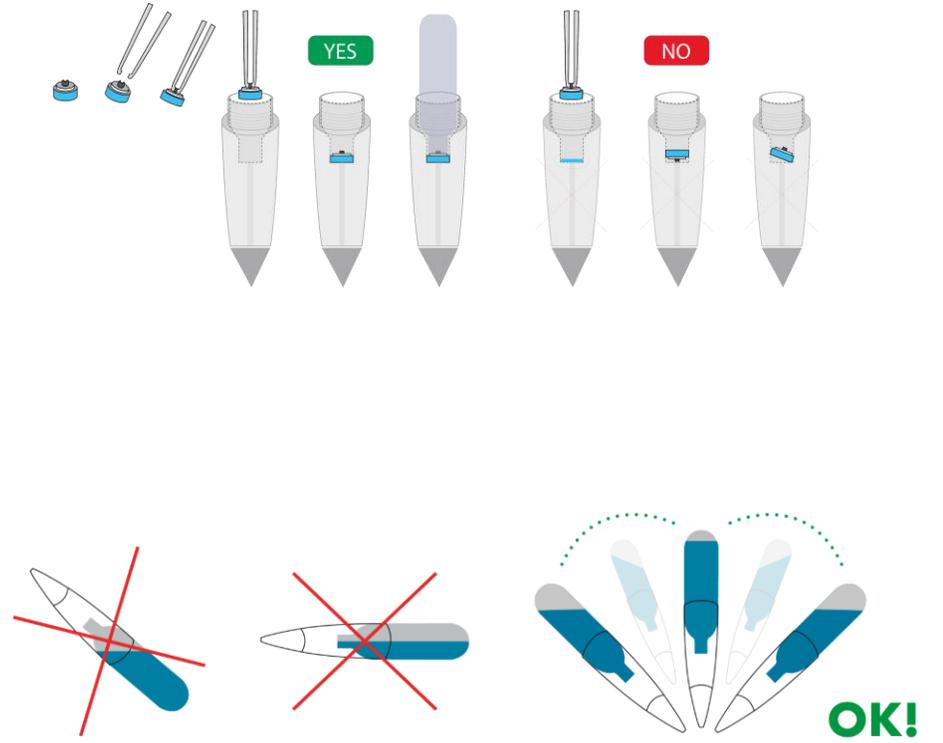

THANK YOU



E-shop



Instagram



Facebook